

The Chronoamperometric and Voltammetric Behaviour of Glutathione at Screen-Printed Carbon Micro-Band Electrodes Modified With Cobalt Phthalocyanine

Kevin C. Honeychurch and John P. Hart[†]

Centre for Research in Biosciences, Faculty of Applied Sciences, University of the West of England, Bristol, BS16 1QY, UK,
[†]corresponding author john.hart@uwe.ac.uk


Abstract Screen-printed carbon electrodes (SPCEs) incorporating the electrocatalyst cobalt phthalocyanine (CoPC) have been successfully used for the manufacture of microband electrodes for the determination of reduced glutathione (GSH). Initially investigations were performed to explore the cyclic voltammetric behaviour of these electrodes with potassium ferrocyanide. It was shown that steady state behaviour occurred which is indicative of radial diffusion at a micro-electrode. Current densities of $2173 \mu\text{Acm}^{-2}$ were obtained compared to $464.4 \mu\text{Acm}^{-2}$ for conventional sized (3 mm x 3 mm) screen-printed electrodes were obtained. At scan rates between 5 and 20 mVs^{-1} no significant increase in current response was observed. The application of these microband CoPC-SPCEs, to the measurement of GSH by both chronoamperometry and cyclic voltammetry was investigated. The chronoamperometric response was found to be linear between $50 \mu\text{M}$ and 8.0 mM with a detection limit of $7.3 \mu\text{M}$ using an applied potential of $+0.25 \text{ V}$ (vs. Ag/AgCl).

Keywords glutathione, cobalt phthalocyanine screen-printed carbon electrodes, voltammetry, chronoamperometry, microband electrodes.


1. Introduction

In a number of recent reviews we have reported on the wide range of applications in which screen-printed carbon electrodes (SPCEs) are presently utilised [1-4]. The majority of these applications have employed working electrodes with geometric areas typically in the square millimetre range. However, to our knowledge there are relatively few studies which have utilised SPCEs for the fabrication of working electrodes in the micrometer (μm) range [5-12]. Such electrodes exhibit a number of analytically advantageous features, such as, improved signal to noise ratios, independence of forced convection and low ohmic drop [13,14]. This can be also be advantageous in a number of application areas, such as *in vitro* cell toxicity studies, as they greatly reduce any perturbation of cell metabolism that may result from *in situ* electrochemically monitoring. The endogenous antioxidant glutathione (GSH) (i) is a frequently monitored compound in such studies [15] providing a good correlation with the redox and detoxification status of the cell [16]. As a reflection of the importance of monitoring GSH, various analytical techniques have been utilised for its determination [17-20]. However, the direct electrochemical of oxidation GSH occurs at relatively high potentials, leading to problems of selectivity in its application; consequently, a number of authors have used some form of electrochemical catalyst to mediate this reaction to more analytically useful potentials [21-27]. Previously we

have reported on the electrochemical behaviour and determination of GSH, at several different carbon based electrodes incorporating the mediator, cobalt phthalocyanine (CoPC) (ii) [24-27].



(i)






(ii)

Scheme (1) structures of (i) glutathione and (ii) cobalt phthalocyanine

This mediated electrochemical reaction occurs via the interaction of the GSH anion, GS^- , (eq. 1) with the native Co^{2+} ion centre of the CoPC molecule [21] forming a Co^+ species

(eq. 2); which can then dissociate to give Co^+ and a glutathione radical (GS^\cdot) (eq.3). The chemically reduced Co^+ can then be readily electrochemically oxidise back to the starting Co^{2+} at potentials close to that of 0 V (eq. 4). The resulting electrocatalytic current generated allows for the measurement of GSH without the application of high positive potentials with their associated interferences and problems of high background currents.



Clearly this is an attractive approach for GSH monitoring and in the present study we have investigated combining this electrocatalytic reaction in conjunction with a microband screen-printed sensor. However, the direct screen-printing of microbands is problematic, as printing of lines thinner than *ca.* 60 μm is generally considered difficult with this technology [28]. However, our group [29-31] have shown a simple alternative method to manufacturing such electrodes from their macro electrodes counterparts.

Our present study is divided into three main sections. We first investigate the possibility of using our macro SPCEs to make microband electrodes in the above manner and then investigate their voltammetric and chronoamperometric behaviour with potassium ferrocyanide and GSH. The conditions were then optimised for the determination of GSH. In the final section, we investigate the possibility of measuring GSH in cell culture medium using constant potential amperometry in unstirred solutions.

2. Experimental

2.1. Chemicals and Reagents

All standard reagents were purchased from Fisher Scientific unless otherwise stated. Deionised water was obtained from a Purite RO200-Stillplus HP System, (Purite Oxon, UK). Separate stock solutions of disodium and monosodium o-phosphate were made at a concentration of 0.2 M by dissolving the appropriate mass of solids in deionised water. These were then titrated to give the required pH. Standard stock solutions of GSH were prepared by dissolving the appropriate mass in sufficient deionised water to give a concentration of 10 mM. Potassium ferrocyanide stock solutions were made in a similar manner. Minimum Essential Medium Eagle (MEM) cell culture media was obtained from Sigma (Poole, UK).

2.2. Apparatus

Voltammetric and chronoamperometric studies were performed with a Pstat10 potentiostat interfaced to a PC for data acquisition via the General Purpose Electrochemical System Software Package (GPES) version 3.4 (Autolab, Windsor Scientific Limited, Slough, Berkshire UK). All experiments were undertaken using a two electrode cell,

consisting of a Ag/AgCl screen-printed counter/pseudoreference electrode and a CoPC-SPCE, as the working electrode supplied by Gwent Electronics Materials Ltd (GEM, Mamhilad, Gwent, UK) printed from C40511D8 ink.

2.3 Microband Formation

The original screen-printed strip is shown in Figure 1a the electrode working area covered with a suitable dielectric (insulating tape, RS Components, Northamptonshire, UK). The end of the working electrode was cut-off perpendicular to the screen-printed carbon track to expose a cross section of the working electrode (figure 1b), sandwiched between the dielectric (insulating tape) and the PVC substrate, hence forming the microband electrode (2 mm x 20 μm) (figure 1c). The working and pseudoreference/counter electrodes were then connected to the potentiostat using a gold clip attached to coaxial cable inserted into the appropriate sockets. A small portion of the working electrode was removed before each measurement, in order to produce new carbon surface. Figure 2 shows an electron micrograph of the microband CoPC SPCE. Here the exposed 20 μm ink layer can be clearly seen, sandwiched between the dielectric (upper) and the PVC substrate (below).

2.4 Voltammetric Procedures

Cyclic voltammograms were recorded with plain 10 ml aliquots of the supporting electrolyte (0.1 M phosphate buffer pH 7) and then with the same solution containing the analyte under investigation. The voltammetric conditions were as follows: initial and final potentials, -0.2 V, with a switching potential of +1.0 V. All experiments were undertaken at 37 $^\circ\text{C}$.

2.5 Optimisation of the Chronoamperometric Potential for Glutathione Detection

In order to deduce the optimum applied potential for calibration studies, chronoamperometric measurements were made at various potentials in a solution containing 5.1 mM GSH 40 s after the application of each potential. This was achieved by transferring a 5 ml aliquot of GSH solution to the cell, stepping the potential from open circuit to -0.2 V and then stepping in 50 mV to a final potential of +0.4 V. The resulting data was used to plot a voltammogram from which we could identify the optimum potential to be used in further chronoamperometric studies.

2.6 Calibration Study on GSH Using Chronoamperometry with Microband CoPC-SPCEs

Calibration solutions were undertaken over the range 0.2 to 25 mM GSH dissolved in 0.1 M pH 7.3 phosphate buffer. Chronoamperograms were recorded initially using a fresh microband CoPC-SPCE for each measurement and 5 ml aliquots of each of the GSH solutions. Each solution was examined by leaving the CoPC-SPCE at open circuit for 5 s before applying a potential of +0.25 V for a period of 60 s. Subsequent studies were made using a method of multiple standard addition at a single microband electrode.

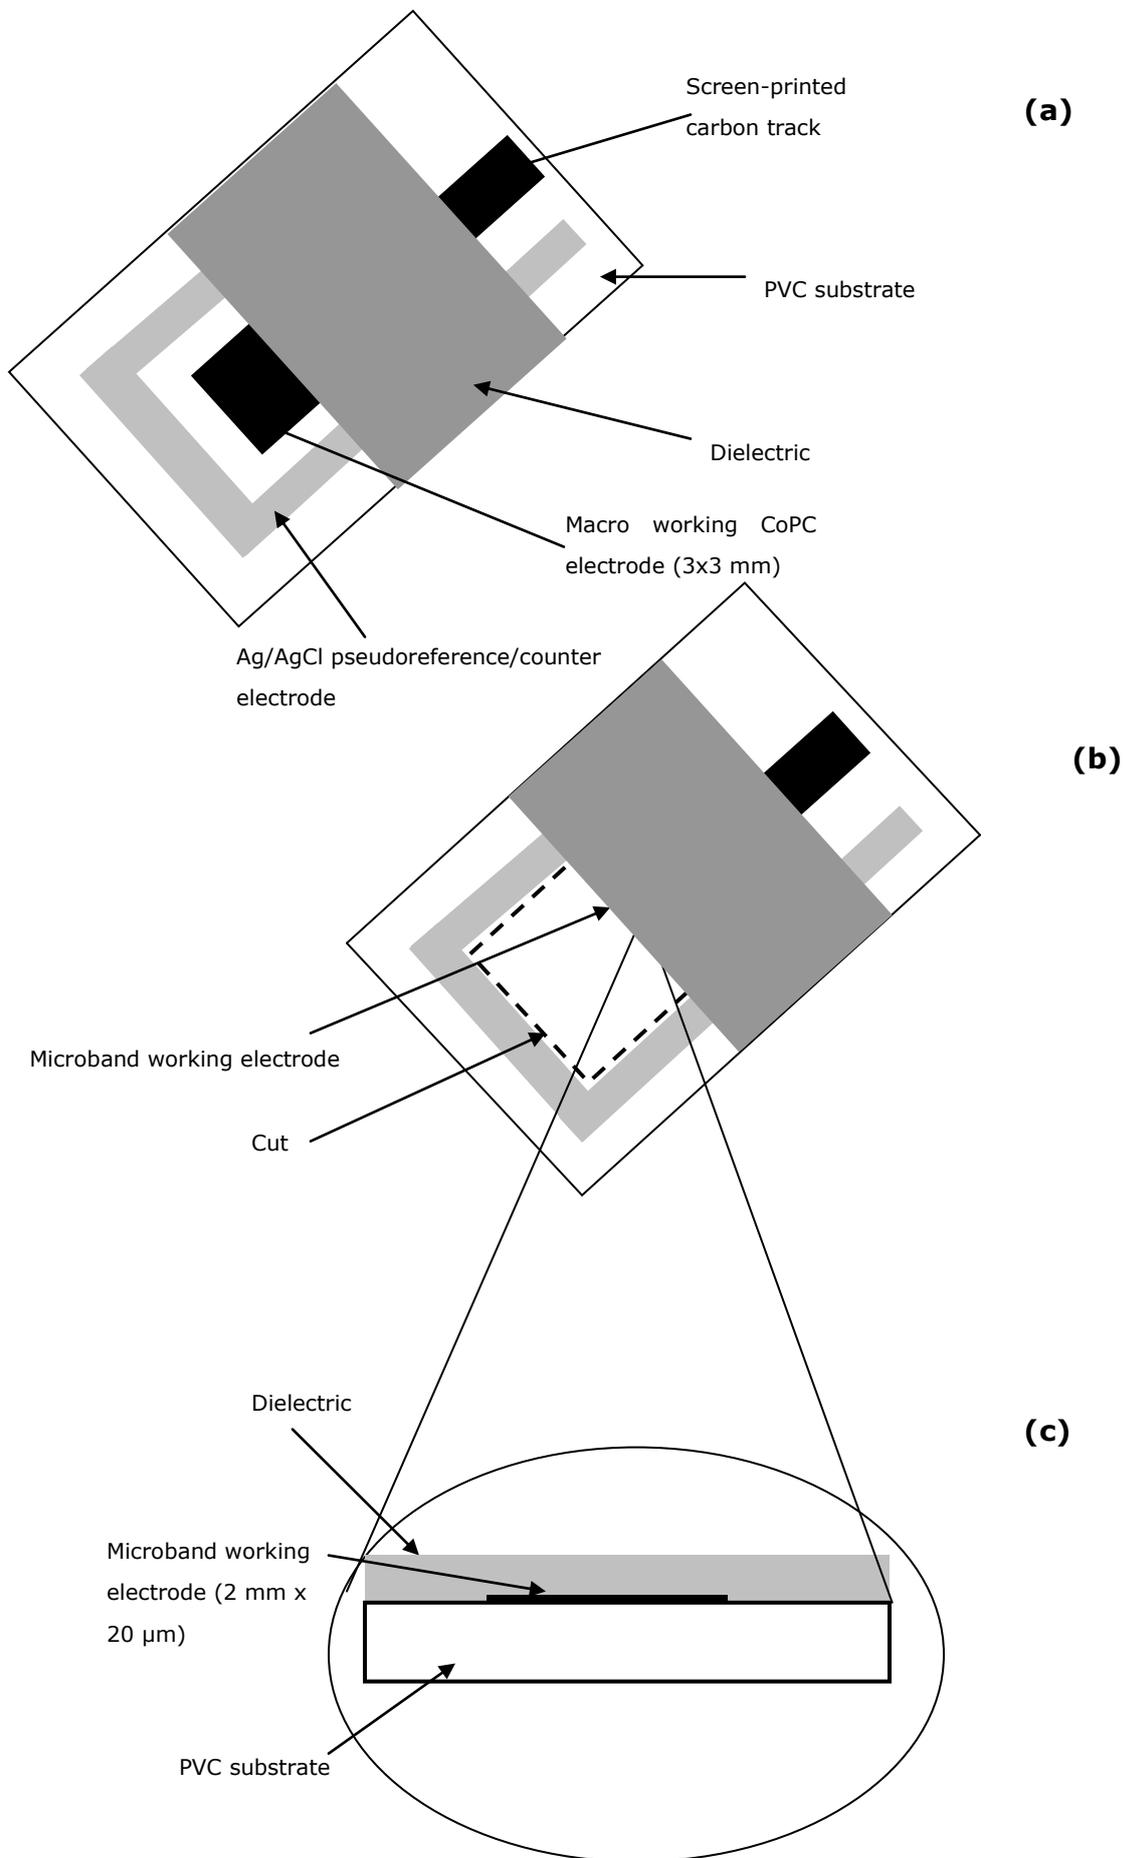


Figure 1 Schematic diagram demonstrating the method for the manufacture of microband SPCEs.

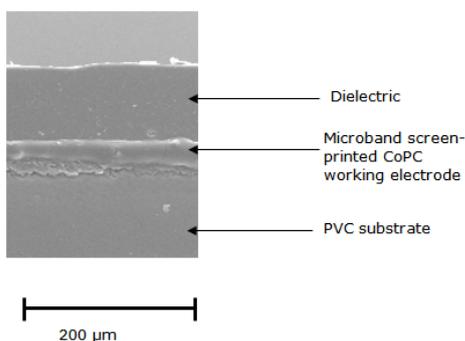


Figure 2. Scanning electron micrograph of a microband CoPC-SPCE.

2.7 Analytical Application

A four mL aliquot of MEM was taken and diluted four mL of 0.2 M phosphate buffer pH 7.3 and a potential of +0.25 V was applied. The system was left to reach a steady-state current (about 100 s), then a total of six 5 μ L additions of a 102 mM GSH standard were made to the cell, using a micropipette, and ensuring steady-state currents between additions. All measurements were made in quiescent solution.

3. Results and Discussion

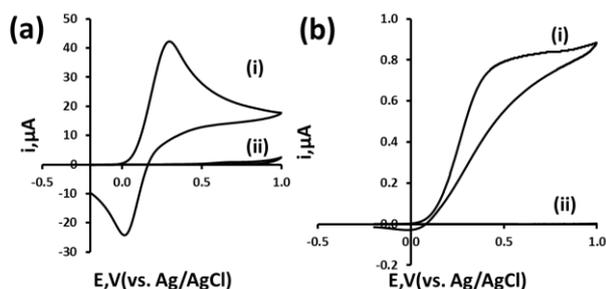


Figure 3. Cyclic voltammograms obtained with 5.1 mM potassium ferrocyanide using a conventional sized CoPC-SPCE: a(i) (area 0.09 cm^2) and microband CoPC-SPCE b(i) (area $4.0 \times 10^{-4} \text{cm}^2$). Cyclic voltammograms for plain 0.1 M phosphate buffer at pH 7.3, obtained for conventional sized CoPC-SPCEs a(ii) and microband CoPC-SPCEs b(ii).

3.1. Cyclic Voltammetric Investigations Using Microband CoPC-SPCEs with Potassium Ferrocyanide

Initial investigations were performed using cyclic voltammetry with our macro and microband CoPC-SPCEs with a 5.1 mM potassium ferrocyanide solution. Figure 3a(i) shows a typical cyclic voltammogram obtained for 5.1 mM potassium ferrocyanide 0.1 M phosphate buffer pH 7.3 solution using a 3x3 mm CoPC-SPCE. A quasi-reversible redox couple is seen with this screen-printed electrode which exhibited typical peak shaped responses. In contrast to this, Figure 3b(i) shows a cyclic voltammogram obtained at our microband electrode. Clearly sigmoidal behaviour is obtained which is a diagnostic test for microelectrode behav-

our. A current density of 2173 μAcm^{-2} was obtained, compared to 464.4 μAcm^{-2} obtained with a 3 x 3 mm macro SPCE. The large increase in current density indicates the elevated mass transport that occurs at the microband electrodes through radial diffusion.

The effect of scan rate on the ferrocyanide oxidation was studied from 5 mVs^{-1} to 20 mVs^{-1} . The voltammetric response of potassium ferrocyanide was found to be independent of scan rate over the range studied, again indicative of radial diffusion and microband electrode behaviour.

3.2. Cyclic Voltammetric Studies using Microband CoPC-SPCEs with Glutathione

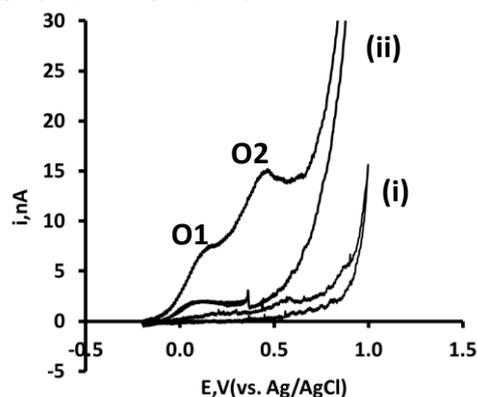


Figure 4. Cyclic voltammograms obtained in the absence (i) and presence (ii) of 1.9 mM GSH in a 0.1 M phosphate buffer at pH 7.3 obtained at a microband CoPC-SPCE using a scan rate of 5 mVs^{-1} .

The cyclic voltammetric behaviour of the proposed microband CoPC-SPCEs (Figure 4) was investigated with a solution containing 1.9 mM GSH in 0.1 M phosphate buffer pH 7.3. Two waves are distinguishable, designated as O1 and O2. We believe that O1 is the result of the electrochemical re-oxidation of Co^+ to Co^{2+} (eq.4), and the additional signal distinguishable at potentials greater than +0.4 V, is believed to result from the further oxidation of Co^{2+} to Co^{3+} , similar to that seen at our macro CoPC-SPCEs under the same voltammetric conditions [25-27]. A scan rate study was performed which demonstrated that the current response for a 1.9 mM GSH solution was independent of scan rate up to at least 20 mVs^{-1} ; this behaviour indicates the presence of radial diffusion and microband electrode behaviour.

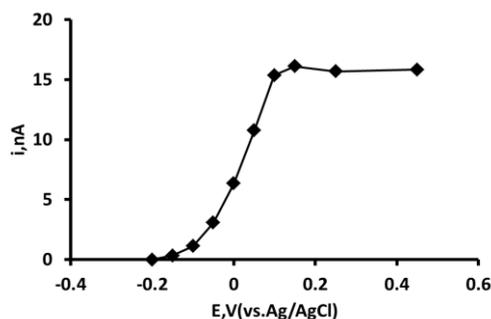


Figure 5. A voltammogram of 5.1 mM GSH in 0.1 M phosphate buffer at pH 7.3 obtained using chronoamperometry in 50 mV steps up to +0.4 V.

3.3. Chronoamperometry

To identify the optimum applied potential for the chronoamperometric measurements of GSH, a voltammogram was obtained by increasing the applied potential from open circuit to +0.4 V in 50 mV steps; Figure 5 shows that the response becomes independent of the applied potential at potentials greater than +0.1 V. From this, it was concluded that an applied potential of +0.25 V would be suitable for further chronoamperometric investigations.

3.4. Calibration Study

Investigations were performed with a series of GSH solutions over the range 0.48 to 4.8 mM; some typical chronoamperograms are shown in Figure 6, each obtained with separate microband electrodes. Current measurements were taken after 20 s and these were plotted against the corresponding concentrations. The resulting plot was linear and the sensitivity of these devices was found to be 0.3 nA/mM. The coefficient of variation obtained at a GSH concentration of 1.66 mM for a single microband electrode was 0.97 % ($n = 3$). Steady state behaviour was observable for all GSH concentrations studied, further indicating the presence of microband behaviour. Additional investigations were made by making multiple measurements at a single microband electrode over the GSH concentration range 50 μM – 25 mM in pH 7.2 0.1 M phosphate buffer. The microband sensor was found to be linear from 50 μM to 8 mM GSH. No enhancement in current response was seen in the presence of forced convection.

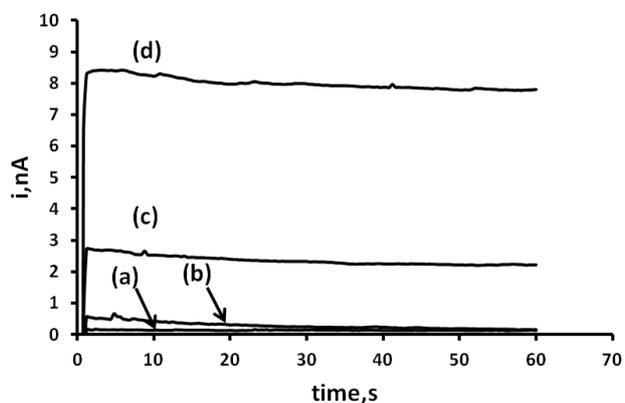


Figure 6. Typical chronoamperograms obtained at microband CoPC-SPCEs using various concentrations of GSH of (a) 0.0, (b) 0.488, (c) 1.95, (d) 4.88 mM. The electrolyte was 0.1 M phosphate buffer at pH 7.3, with an applied potential of +0.25 V.

3.5. Analytical Application

The behaviour of GSH in MEM was investigated using the optimised assay. MEM is known to be GSH free and only a small baseline current is observable using an applied potential of +0.25 V (Figure 7). The addition of 63.8 μM GSH to the system results in a rapid current increase resulting from

the oxidation of GSH at the CoPC microband SPCE. Further additions of this standard resulted in a linear increase in current over the range examined with an associated $R^2 = 0.999$ (Figure 8). An estimated detection limit of 7.3 μM was calculated based on a signal-to-noise ratio of three.

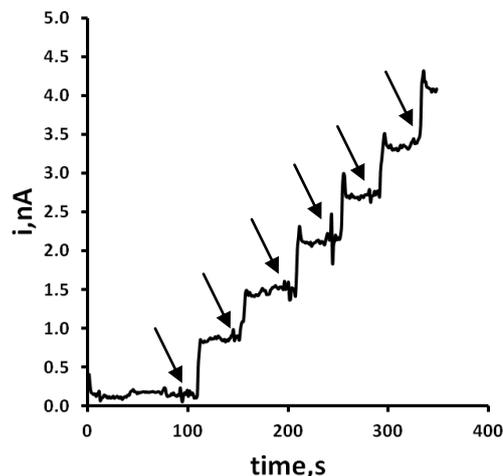


Figure 7. Chronoamperometric investigations of GSH at a microband CoPC-SPCE electrode in MEM dilute 1:1 with 0.2 M phosphate buffer solution, pH 7.4 at 37 °C. Arrows represent additions of 5 μL 102 mM GSH into 8 mL quiescent (stirred only to mix for 10 s).

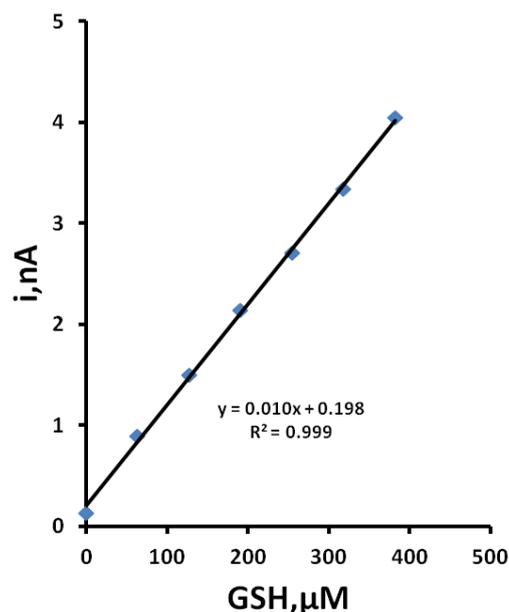


Figure 8. Standard addition plot for GSH in MEM. Conditions as described in Figure 7.

4. Conclusion

To our knowledge, the present study is first report on the development of microband electrodes based on SPCEs modified with the electrocatalyst CoPC for the determination of GSH. We have demonstrated that these electrodes show behaviour which is characteristic of microelectrodes for both GSH and potassium ferrocyanide. Initial cyclic voltammetric investigations using 5 mM ferrocyanide in phosphate buffer solution with our macro (3x3 mm) CoPC-SPCEs showed typical diffusion control behaviour. However, voltammograms for this species obtained with our microband CoPC-SPCEs developed in this study showed much greater current density and a sigmoidal anodic wave with no cathodic response, typical of microelectrode behaviour. Further cyclic voltammetric investigations for the same microband electrodes, using 7 mM GSH in phosphate buffer at several different scan rates showed the response to be independent of scan rate, indicative of microband behaviour.

Chronoamperometry was performed with these microband CoPC-SPCEs at different concentrations of GSH. Steady state behaviour was observed for each concentration investigated over the range 0 to 25 mM. The steady state current was found to be linearly related with GSH concentration over the range 50 μ M-8 mM in 0.1 M phosphate buffer pH 7.2, at an applied potential of +0.25 V (vs. Ag/AgCl). This behaviour is important as it demonstrates possibility of monitoring GSH continuously which could be exploited for cell metabolism studies [32]. Future work will focus on such studies. Our performance characteristics compare well with those previously reported [24-27]. Pereira-Rodrigues *et al* [33] recently reported a similar linear range of 80 μ M to 1 mM at a CoPC modified graphite electrode. However, these devices could not readily be mass produced at low cost to create disposable devices for cell metabolism studies. In addition, as they are macro-sized devices they would perturb the cell behaviour; therefore they would be unsuitable for the proposed application. Other reports [24-27] have described macro-sized CoPC-SPCEs for GSH determination with similar linear ranges to that obtained with our proposed microband CoPC-SPCE. However, as previously mentioned, these devices would be unsuitable for cell metabolism studies owing to the higher consumption of GSH. Importantly, microband CoPC-SPCEs would consume very little GSH and the solutions do not need stirring to give steady state currents as mass transport occurs by radial diffusion.

ACKNOWLEDGEMENT

The authors would like to thank the HEFCE for funding. They are grateful to Gwent Electronic Materials Ltd. for supplying the screen-printed carbon electrodes. Dr. Jins-heng Xu is thanked for the gift of the cell culture media and Dr. David Patton for his assistance with the SEM analysis.

REFERENCES

- [1] J.P. Hart, A. Crew, E. Crouch, K.C. Honeychurch, R.M. Pemberton, 2007, Recent developments in screen-printed carbon electrode sensors/biosensors for electrochemical analysis. Chapter 23 in *Comprehensive Analytical Chemistry*, vol. 49, Eds. S. Alegret, A. Merkoci, R.M. Elsevier B.V., Amsterdam, pp. 497-557.
- [2] J.P. Hart, A.K. Abass, K.C. Honeychurch, R.M. Pemberton, S.L. Ryan, R. Wedge, 2003, Sensors/biosensors, based on screen-printing technology for biomedical applications, *Indian Journal of Chemistry Section A-Inorganic Bio-Inorganic Physical Theoretical & Analytical Chemistry*, 42, 709-718.
- [3] J.P. Hart, A. Crew, E. Crouch, K.C. Honeychurch, R.M. Pemberton, 2004, Some recent designs and developments of screen-printed carbon electrochemical sensors/biosensors for biomedical, environmental and industrial analyses, *Anal. Lett.* 37, 789-830.
- [4] K.C. Honeychurch and J.P. Hart, 2003, Screen-printed electrochemical sensors for monitoring metal pollutants, *TrAC*, 7/8, 456-469.
- [5] J.-L. Chang and J.-M. Zen, 2006, Fabrication of disposable ultramicroelectrodes: Characterization and applications, *Electrochem. Commun.* 8, 571-576.
- [6] D.H. Craston, C.P. Jones, D.E. Williams, N. Elmurr, 1991, Microband Electrodes Fabricated By Screen Printing Processes - Applications in Electroanalysis, *Talanta*, 38, 17-26.
- [7] D.E. Williams, K. Ellis, A. Colville, S.J. Dennison, G. Laguillo, J. Larsen, 1997, Hydrodynamic modulation using vibrating electrodes: Application to electroanalysis, *J. Electroanal. Chem.* 432, 159-169.
- [8] M. Rochelet-Dequaire, B. Limoges P. Brossier, 2006, Sub-femtomolar electrochemical detection of target DNA by catalytic enlargement of the hybridized gold nanoparticle labels, *Analyst*, 131, 923-929.
- [9] F.J. Rawson, W.M. Purcell, J. Xu, D.C. Cowell, P.R. Fielden, N. Biddle, J.P. Hart, 2007, Fabrication and Characterisation of Novel Screen-Printed Tubular Microband Electrodes, and Their Application to the Measurement of Hydrogen Peroxide, *Electrochim. Acta*, 52, 7248-7253.
- [10] L. Authier, C. Grossiord, P. Brossier, B. Limoges, 2001, Gold Nanoparticle-Based Quantitative Electrochemical Detection of Amplified Human Cytomegalovirus DNA Using Disposable Microband Electrodes, *Anal. Chem.* 73, 4450-4456.
- [11] J.C. Ball, D.L. Scott, J.K. Lumpp, S. Daunert, J. Wang, L.G. Bachas, 2000, Electrochemistry in Nanovials Fabricated by Combining Screen Printing and Laser Micromachining, *Anal. Chem.* 72, 497-501.
- [12] A. Tizzard, J. Webber, R. Gooneratne, R. John, J. Hay, N. Pasco, 2004, MICREDOX: application for rapid biotoxicity assessment, *Anal. Chim. Acta*, 522, 197-205.
- [13] A.M. Bond, 1994, Past, Present and Future Contributions of Microelectrodes to Analytical Studies Employing Voltammetric Detection - A Review, *Analyst* 119, R1-R21.
- [14] X. Xie, D. Stueben, Z. Berner, 2005, The application of microelectrodes for the measurements of trace metals in water, *Anal. Lett.* 38, 2281-2300.
- [15] H. Hahn, C.W. Huck, M. Rainer, M. Najam-ul-Haq, R. Bakry, T. Abberger, P. Jennings, W. Pfaller, G.K. Bonn, 2007, Analysis of glutathione in supernatants and lysates of a human proximal tubular cell line from perfusion culture upon

intoxication with cadmium chloride by HPLC and LC-ESI-MS, *Anal. Bioanal. Chem.* 388, 1763–1769.

- [16] J.P. Richie, P. Abraham, Y. Leutzinger, 1996, Long term stability of blood glutathione and cysteine in humans, *Clin. Chem.* 42, 1100–1105.
- [17] J.C. Harfield, C. Batchelor-McAuley, R.G. Compton, 2012, Electrochemical determination of glutathione: a review, *Analyst*, 137, 2285–2296.
- [18] D. Húska, O. Zitka, V. Adam, M. Beklová, S. Křížková, L. Zeman, A. Horna, L. Havel, J. Zehnálek, R. Kizek, 2007, A sensor for investigating the interaction between biologically important heavy metals and glutathione, *Czech J. Anim. Sci.* 52, 37–43.
- [19] W.B. Jakoby, O.W. Griffith, 1987, Sulfur and Sulfur Amino Acids, *Methods in Enzymol.* 143 and references therein.
- [20] R. Rossi, A. Milzani, I. Dalle-Donne, D. Giustarini, L. Lusini, R. Colombo, P. Di Simplicio, 2002, Blood Glutathione Disulfide: In Vivo Factor or in Vitro Artifact? *Clin. Chem.* 48, 742–753.
- [21] J.H. Zagal, 1992, Metallophthalocyanines as Catalysts in Electrochemical Reactions, *Coord. Chem. Rev.* 119, 89–136.
- [22] F. Ricci, F. Arduini, A. Amine, D. Moscone, G. Palleschi, 2004, Characterisation of Prussian blue modified screen-printed electrodes for thiol detection, *J. Electroanal. Chem.* 563, 229–237.
- [23] P.C. White, N.S. Lawrence, J. Davis, R.G. Compton, 2002, Electrochemical Determination of Thiols: A Perspective, *Electroanalysis*, 14, 89–98.
- [24] S.A. Wring, J.P. Hart, B.J. Birch, 1992, Development of an Amperometric Assay for the Determination of Reduced Glutathione, using Glutathione-Peroxidase and Screen-printed Carbon Electrodes Chemically Modified with Cobalt Phthalocyanine, *Electroanalysis*, 4, 299–309.
- [25] S.A. Wring, J.P. Hart, B.J. Birch, 1991, Voltammetric Behaviour of Screen-Printed Carbon Electrodes, Chemically Modified With Selected Mediators, and their Application as Sensors for the Determination of Reduced Glutathione, *Analyst*, 116, 123–129.
- [26] S.A. Wring and J.P. Hart, B.J. Birch, 1989, Development of an Improved Carbon Electrode Chemically Modified with Cobalt Phthalocyanine as a Re-usable Sensor for Glutathione, *Analyst*, 114, 1563–1570.
- [27] S.A. Wring, J.P. Hart, L. Bracey, B.J. Birch, 1990, Development of screen-printed carbon electrodes modified with cobalt phthalocyanine, for electrochemical sensor applications, *Anal. Chim. Acta*, 231, 203–212.
- [28] A. Hobby, *Screen Printing for the Industrial User*, DEK Printing Machines Ltd. March 1997.
- [29] K.C. Honeychurch, S. Al-Berezanchi, J.P. Hart, 2011, The voltammetric behaviour of lead at a microband screen-printed carbon electrode and its determination in acetate leachates from glazed ceramic plates, *Talanta*, 84, 717–723.
- [30] F.J. Rawson, W.M. Purcell, J. Xu, R.M. Pemperton, P.R. Fielden, N. Biddle, J.P. Hart, 2009, A microband lactate biosensor fabricated using a water-based screen-printed carbon ink, *Talanta*, 77, 1149–1154.
- [31] R.M. Pemperton, R. Pittson, N. Biddle, J.P. Hart, 2009, Fabrication of microband glucose biosensors using a screen-printing water-based carbon ink and their application in serum analysis, *Biosens. Bioelectron.* 24, 1246–1252.
- [32] J. Xu, M. Ma, W.M. Purcell, 2003, Biochemical and functional changes of rat liver spheroids during spheroid formation and maintenance in culture: II. nitric oxide synthesis and related changes, *J. Cell. Biochem.*, 15, 90, 1176–1185.
- [33] N. Pereira-Rodrigues, R. Cofré, J.H. Zagal, F. Bedioui, 2007, Electrocatalytic activity of cobalt phthalocyanine CoPc adsorbed on a graphite electrode for the oxidation of reduced L-glutathione (GSH) and the reduction of its disulfide (GSSG) at physiological pH, *Bioelectrochemistry*, 70, 147–154.